


Blood Ammonia Meter

PocketChem BA

PA-4140

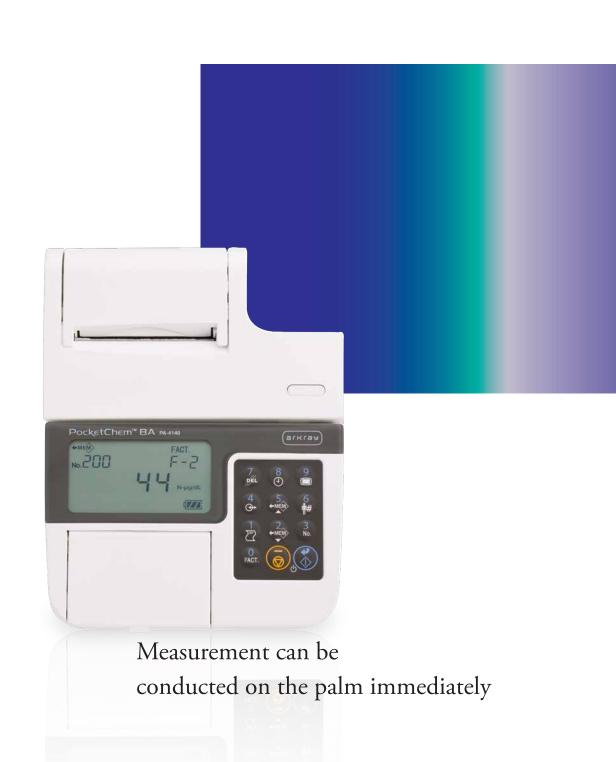

Blood Ammonia Meter

PocketChem BA

PA-4140



Whole-blood measurement

PocketChem BA realizes whole blood measurement without pretreatment. The level of blood ammonia that is susceptible to room temperature can be measured right after collecting blood.

Small sample volume

Required amount for measurement is only $20\mu L$. No special collection tube is necessary.

Palm size and compact design

The weight of the analyzer is approx. 150 g (not including batteries). The weight of the palm-sized analyzer is just 150 g.

Detachable printer

A printer (optional) can be detached from the analyzer. Hard copy of measurement result can be obtained if you connect a printer to analyzer. Printer and AC adapter can be used commonly with Comapct Urine Analyzer PU-4010.

Battery driven

Analyzer can be operated by two AA batteries or with AC adapter.

* The AC adapter is needed when using the printer.

Easy-to-maintain

All what you need to clean daily is the removable strip holder.Implementation of LED for light source eliminated a complicated lamp replacement.

Temperature compensation

Built-in temperature sensor automatically compensates for temperature in the range of $10 - 35^{\circ}$ C.

Data management function

Up to 50 measurement results can be memorized. Using serial communication function (RS-232C), measurement results can be transferred to PC.

Performing a test



Drop a blood sample on the test strip and press start key.



When buzzer sounds after 180 seconds, rip off the spacer part of the test strip.



Place the test strip with the spacer part ripped off on the test strip tray.



Measurement result will be shown.



Hard copy of measurement result can be obtained by connecting a printer.

PocketChem BA size




 $Meter: 124 \ (width) \times 85 \ \ (depth) \times 38 \ (height) \ mm$ $Printer: 125 \ (width) \times 133 \ (depth) \times 36 \ (height) \ mm$

The exclusive test strip

Ammonia Test Kit II

Dry chemistry based on a microdiffusion method provides high-precision measurement with whole blood.



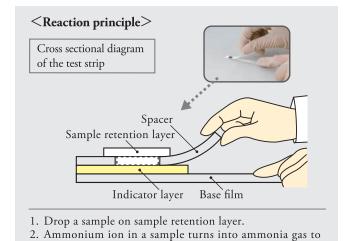

3. Indicator layer reacts to ammonia gas to give a color.

4. Measure the reflected light to obtain the level of color


pass through the spacer.

with PocketChemBA.

PA-4140 specifications Whole blood AMMONIA TEST KIT II Test strip Blood ammonia concentration Measurement item 10 to 400 N - μg / dL Measurement range Measurement principle Test strip, Single wavelength reflectance method Single wavelength LED (635 nm) Measurement wavelength Dropping with pipette Sample supply method Reaction time Approx. 3 minutes and 20 seconds per test Max. 10 seconds Warm-up time Normal measurement, continuous measurement and check Measurement types measurement LCD Test results for 50 samples Memory capacity RS-232 C compliant External output Thermal compensation Automatic compensation using a built-in temperature sensor Temperature: 10-35 °C; Humidity: 25 - 85 % RH Operating environment Dimensions Instrument: 124 (W) \times 85 (D) \times 38 (H) mm Approx. 150 g (not including batteries) Weight ument: Two AA batteries or AC adapter 7.5 VDC 3A

Power supply	Instrument: I wo AA batteries of AC adapter 7.5 VDC 3A
Power consumption	Battery power: 0.15 W (AC power: 4 W)
Printer specifications	
Printer	Thermal line printer
Printer paper	High color development thermal paper (W 58 mm × φ 26 mm)
Dimensions	125 (W) × 133 (D) × 36 (H) mm
Weight	180 g (not including printer paper)
Power supply	AC adapter 7.5 VDC 3A
Power consumption	20 W

Compact Urine Analyzer PocketChem UA



Legal manufacturer arkray factory, Inc.

1480 Koji Konan-cho, Koka, Shiga-ken 520-3306, JAPAN

European representative arkray europe, B.V.

Prof. J.H. Bavincklaan 2, 1183 AT Amstelveen, THE NETHERLANDS https://www.arkray.eu/english/

*Designs and specifications may be changed without prior notice.

arkray global business, inc.

Yousuien-nai, 59 Gansuin-cho, Kamigyo-ku, Kyoto 602-0008, JAPAN TEL +81-75-662-8979 FAX +81-75-431-1202